

Gelweave™

Thoracic and Thoracoabdominal Graft Geometries



Ante-Flo



Extra Length
Ante-Flo with
Offset Branch



4 Branch Plexus



Valsalva™



Siena™



Gelweave
Trifurcate Arch




Thoracoabdominal
Trifurcate

Ante-Flo

Aortic Arch Applications

- Antegrade flow made easy by the side branch for
 - Minimized circulatory arrest time and earlier patient re-warming¹
 - Lower risk of neurological deficits²
 - Reduced chance of perfusing aortic false lumen¹
- Convenience and graft integrity maintained

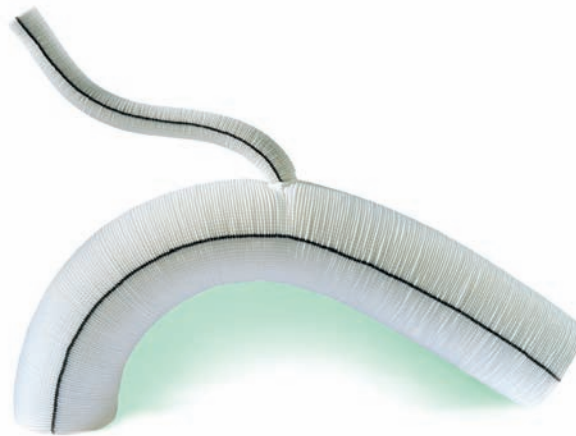

Bore size mm	Usable Length cm	Cat No.
20	40 x 1 @ 15	734020/8
22	40 x 1 @ 15	734022/8
24	40 x 1 @ 15	734024/8
26	40 x 1 @ 15	734026/8
28	40 x 1 @ 15	734028/8
30	40 x 1 @ 15	734030/8
32	40 x 1 @ 15	734032/8
34	40 x 1 @ 15	734034/8

Side Branch Diameter 8mm

Also available with

20cm usable length large bore section - Cat Nos. 732022/8 to 732034/8

10mm diameter perfusion side branch - Cat Nos. 734020/10 to 734034/10 and 732022/10 to 732034/10

See back for references.

Extra Length Ante-Flo with Offset Branch

Aortic Arch Repair

Standard Ante-Flo applications and left subclavian artery repair



Bore size mm	Cat No.
22	735022/8S
24	735024/8S
26	735026/8S
28	735028/8S
30	735030/8S
32	735032/8S

Perfusion side branch diameter 8mm

Body and perfusion side branch usable lengths 50cm and 15cm respectively

See back for references.

Pre-curved Ante-Flo

Aortic Arch Applications

Additional features and benefits to that of the standard Ante-Flo

- Unique pre-curved design
- Closely matches aortic arch anatomy
- Potential for reduced kinking



Bore size mm	Cat No.
22	735022ST/8A
24	735024ST/8A
26	735026ST/8A
28	735028ST/8A
30	735030ST/8A
32	735032ST/8A
34	735034ST/8A

Perfusion side branch diameter 8mm

Body and perfusion side branch usable lengths 50cm and 15cm respectively

See back for references.

Pre-curved Graft

Aortic Arch Repair

- Unique pre-curved design
- Closely matches aortic arch anatomy
- Potential for reduced kinking



Bore size mm	Cat No.
22	735022ST
24	735024ST
26	735026ST
28	735028ST
30	735030ST
32	735032ST
34	735034ST

Product usable length 50cm

See back for references.


Plexus

Aortic Arch and Associated Major Artery Replacement

- 3 or 4 branch designs
- Antegrade flow made easy by the perfusion side branch may offer
 - Reduced incidence of temporary neurological deficits²
 - Preventive effect against embolic stroke³
 - Potential for reduced operating time⁴
- Convenience and graft integrity maintained



3 Branch

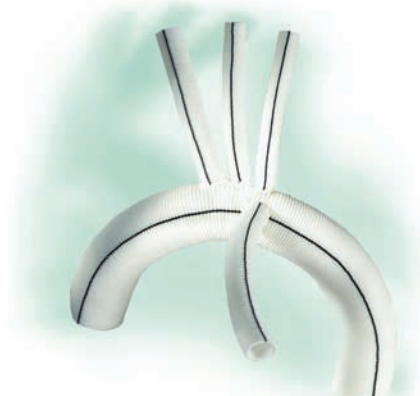

4 Branch

Bore size mm	Cat No.
20	73201088
22	73221088
24	73241088
26	73261088
28	73281088
30	73301088
32	73321088
34	73341088

Bore size mm	Cat No.
20	73201088/8
22	73221088/8
24	73241088/8
26	73261088/8
28	73281088/8
30	73301088/8
32	73321088/8
34	73341088/8

Body and branch usable lengths 40cm and 15cm respectively
Arch branch diameters 10 x 8 x 8mm. Side branch diameter 8mm

Also available with a 10mm diameter perfusion side branch - Cat Nos. 73201088/10 to 73341088/10
See back for references.

Siena™ Collared Grafts with Radiopaque Markers

Aortic Arch Applications

- Primarily indicated for first stage elephant trunk procedures⁵
- The collar compensates for diameter mismatch between distal aorta and graft,
 - Reducing tension on the distal anastomosis⁵
 - Potentially reducing the risk of aneurysm rupture before second stage repair⁵
- Side branch permits antegrade perfusion^{1,2}


Siena™ Ante-Flo



Bore Size mm	Graft Body		Cat No.
	Usable Length cm		
20	50		735020/8RM
22	50		735022/8RM
24	50		735024/8RM
26	50		735026/8RM
28	50		735028/8RM
30	50		735030/8RM
32	50		735032/8RM
34	50		735034/8RM

- Perfusion side branch offset at 30° in a horizontal plane to the body of the graft - bore size 8mm - length 15cm.
- Also available with a 10mm perfusion branch - Catalogue Numbers 735020/10RM - 735034/10RM

Siena™ 4 Branch Plexus

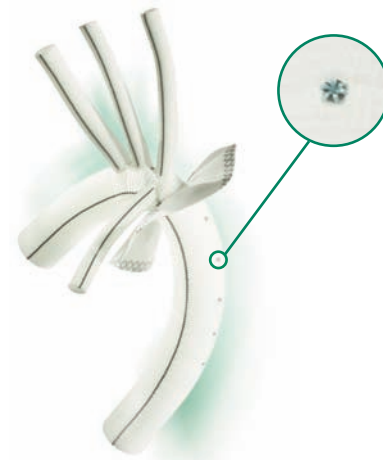

Bore Size mm	Graft Body		Cat No.
	Usable Length cm		
20	50		73201088/8RM
22	50		73221088/8RM
24	50		73241088/8RM
26	50		73261088/8RM
28	50		73281088/8RM
30	50		73301088/8RM
32	50		73321088/8RM
34	50		73341088/8RM

- Side branches - bore sizes 10 x 8 x 8mm - length 15cm
- Perfusion side branch offset at 30° in a horizontal plane to the body of the graft - bore size 8mm - length 15cm
- Also available with a 10mm perfusion side branch - Catalogue Numbers 73201088/10RM - 73341088/10RM

For all designs:

- Overall length 50cm.
- Graft proximal end to collar 20cm.
- Collar to graft distal end 30cm.
- Relaxed distance between markers 2cm.

Siena™ Collared Grafts are made from: **Gelweave™** - main body and side branches, **Gelseal™** - collar. See back for references.

Valsalva™

Proximal Thoracic Aorta Replacement

- Unique aortic graft design for valve sparing or Bentall procedures
- Closely matches aortic root anatomy⁶
- Mimics natural response of the sinuses of Valsalva⁷
- Potential for
 - Increased valve leaflet longevity⁸
 - Reduced tension on the coronary arteries



Bore size mm	Maximum Skirt Diameter mm	Body Length cm	Skirt Length mm	Collar Length mm	Cat No.
24	32	15	24	10	730024ADP
26	34	15	26	10	730026ADP
28	36	15	28	10	730028ADP
30	38	15	30	10	730030ADP
32	42	15	32	10	730032ADP
34	44	15	34	10	730034ADP

Gelweave™

Trifurcate Arch Graft

Aortic Arch Applications

- Shortens hypothermic circulatory arrest times⁹
- Minimizes cerebral ischemia¹⁰
- No touch technique - reduces the risk of embolization¹⁰
- Minimizes adverse outcomes⁹
- Complements first stage elephant trunk repair⁹



Bore Size (mm)		Cat No.
Body	Branches	
12	8	732012/8X2
12	10	732012/10X2
14	8	732014/8X2
14	10	732014/10X2


Graft body usable lengths 20cm
Branch usable lengths 10cm

See back for references.

Trifurcate

Thoracoabdominal Aortic Reconstruction

- Sequential visceral and renal artery replacement¹²
- Permits short visceral, renal and spinal ischemic times¹²
- Offers low rates of end organ ischemic damage and paraplegia¹²

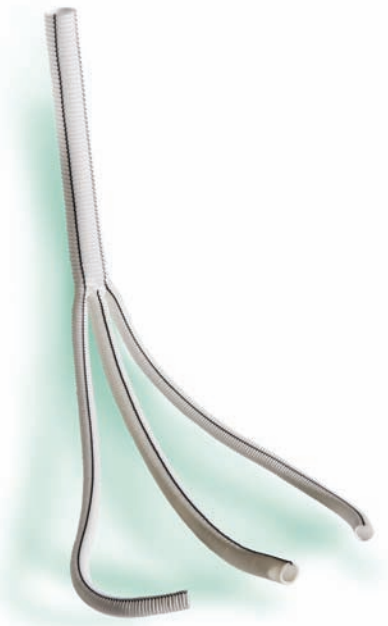

Cat No	Bore Size (mm)			Usable Length (cm)
	Body	Central Branch	Lateral Branches	
731206/7	12	7	6	45
731407/7	14	7	7	45
731608/7	16	7	8	45

Graft body usable lengths 15cm
Branch usable lengths 30cm

See back for references.

References

1. Havel M. *et al.* **Operative Management of Aortic Aneurysms Using Profound Hypothermia & Circulatory Arrest.** *International Congress on Thoracic & Thoracoabdominal Aortic Aneurysm 12-14 June 1994*; 23-26.
2. Ehrlich M. *et al.* **The Use of Profound Hypothermia and Circulatory Arrest in Operations on the Thoracic Aorta.** *European Journal of Cardiothoracic Surgery* 1997; **11**: 176-181.
3. Shiiya N. *et al.* **Surgical Management of Atherosclerotic Aortic Arch Aneurysms Using Selective Cerebral Perfusion: 7-Year Experience in 52 Patients.** *European Journal of Cardiothoracic Surgery* 2000, **17**: 266-271.
4. Adachi H *et al.* **Usefulness of a New Branched Sealed Graft for the Replacement of the Aortic Arch.** *Japanese Journal for Artificial Organs* 1997; **26 3**: 624-628.
5. Neri E. *et al.* **The “Elephant Trunk” Technique Made Easier.** *Ann Thorac Surg* 2004; **78**: 17-8.
6. De Paulis R. *et al.* **A New Aortic Dacron Conduit for Surgical Treatment of Aortic Root Pathology.** *Ital Heart J* 2000; **1 (7)**: 457-463.
7. De Paulis R. *et al.* **Opening and Closing Characteristics of the Aortic Valve After Valve-Sparing Procedures Using a New Aortic Root Conduit.** *Ann Thorac Surg* 2001; **72**: 487-94.
8. De Paulis R. *et al.* **Analysis of Valve Motion After the Reimplantation Type of Valve-Sparing Procedure (David I) with a New Aortic Root Conduit.** *Ann Thorac Surg* 2002; **74**: 53-57.
9. Strauch JT. *et al.* **Technical Advances in Total Aortic Arch Replacement.** *Ann Thorac Surg* 2004; **77**: 581-590.
10. Spielvogel D. *et al.* **Aortic Arch Reconstruction Using a Trifurcated Graft.** *Ann Thorac Surg* 2003; **75**: 1034-1036.
11. Personal Communication (Professor J S Coselli, 23 September 2003).
12. Ballard J. *et al.* **Type III and IV Thoracoabdominal Aortic Aneurysm Repair: Results of a Trifurcate/Two Graft Technique.** *Journal of Vascular Surgery Vol 36, No. 2, August 2002.*



Distributed in the US by:
Terumo Cardiovascular Systems
6200 Jackson Road
Ann Arbor MI 48103-9300
Customer Service: 888-758-8000
Fax: 800-292-6551
www.terumo-cvs.com



Manufactured by:
Vascutek, a **TERUMO** Company
Newmains Avenue, Inchinnan
Renfrewshire PA4 9RR, Scotland, UK
Tel: (+44) 141-812-5555
Fax: (+44) 141-812-7170
www.vascutek.com